

## Wuhan HealthCare Biotechnology Co., Ltd.

LeaderBuilding #8, Optics Valley Precision Medicine Industry Park Phase 1,<br/>#9 Gaokeyuan 3rd Road, East Lake High-Tech Zone. Zip Code 430206, Wuhan, Hubei, China.Tel#: +86(027)8757-0662 E-mail: cs@healthcare-biotech.com | Website: www.healthcare-biotech.com

### Product Cat. No.: FP-085

### For Clinical Diagnosis & Scientific Research.

## PTEN gene deletion probe reagent Instructions Manual


[Product Name] PTEN gene deletion probe reagent. [Package specification] 10Tests /box.

#### [Product introduction]

The kit uses orange fluorescein to label PTEN probe and green fluorescein to label CEP10 probe. PTEN/CEP10 probe can be combined with the target detection site by in situ hybridization.

#### [Product Main Components]

The kit consists of PTEN/CEP10 dual color probe, as shown in Table 1.

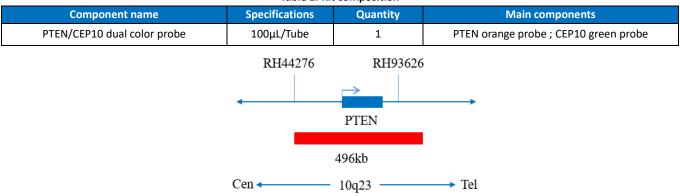

#### Table 1: Kit composition

#### [Storage conditions & Validity]

Keep sealed away from light at -20°C±5°C. The product is valid for 12 months. Avoid unnecessary repeated freezing and thawing that should not exceed 10 times. After opening, within 24 hours for short-term preservation, keep sealed at 2~8°C in dark. For long-term preservation after opening, keep the lid sealed at -20°C±5°C away from light. The kit was transported below 0°C.

#### [Applicable Instruments]

Fluorescence microscope imaging system, including fluorescence microscope and filter set suitable for DAPI (367/452), green (495/517) and orange (547/565).

#### [Sample Requirements]

1. Applicable specimen type: paraffin embedded specimen of surgical resection or biopsy tissue.

2. The tissue in vitro should be fixed with 4% neutral formaldehyde fixative within 1 hour. After the tissue is fixed, it is often dehydrated and embedded in paraffin.





## Wuhan HealthCare Biotechnology Co., Ltd.

 Leader
 Building #8, Optics Valley Precision Medicine Industry Park Phase 1,

 #9 Gaokeyuan 3rd Road, East Lake High-Tech Zone. Zip Code 430206, Wuhan, Hubei, China.

 Tel#: +86(027)8757-0662 E-mail: cs@healthcare-biotech.com

 Website: www.healthcare-biotech.com

#### [Instructions]

#### 1. Hybridization pretreatment

Baking: Slides heating at 80°C for 30min or 65°C for 2h or overnight.

Dewaxing: According to the customer laboratory protocol (Commonly with Xylene for 15min).

Hydration: Take out the slides and put them respectively into 100%, 85% and 70% EtOH at room temperature for 3 minutes each.

Take out the slides, and immerse them in deionized water for 3 minutes. Remove the excess of water on the slides by air-drying.

Permeation: Immerse the slides in deionized water at 100°C and boil continuously for 20-40 minutes (Conventional 20min). Remove the excess of water on the slides by air-drying.

Digestion: Protease enzymic digestion at 37°C for 10-40 minutes. Mix the protease work buffer (50mmol HCl) and the 10x protease solution (Pepsin concentration 5%) in a proportion of 9:1 to prepare the enzymatic digestion solution.

Washing: Wash with 2xSSC at room temperature for 5 minutes.

Dehydration: Take out the slides and dehydrate in 70%, 85%, and 100% gradient ethanol at room temperature for 2 minutes each time. Remove the excess of EtOH solution on the slides by air-drying.

#### 2. Denaturing hybridization

The following operations should be carried out in the dark room.

(1) Take out the probe, let it stand at room temperature for 5min, turn it upside down with force, mix the probe well, centrifuge it briefly (do not vibrate with vortex apparatus), drop 10 $\mu$ l into the hybridization area of the cell drop, cover the 22mm×22mm cover glass immediately, the probe should be evenly spread under the cover glass without bubbles, and seal the edge with rubber (the edge sealing must be thorough to prevent the dry slide from affecting the test results in the hybridization process).

(2) Place the glass slide in the hybridization instrument, denature at  $85^{\circ}$ Cfor 5 min (the hybridizer should be preheated to  $85^{\circ}$ C) and hybridized at  $42^{\circ}$ Cfor 2-16h.

#### 3. Washing

The following operations should be carried out in a dark room.

(1) Carefully remove the sealing glue around the cover glass with tweezers to avoid sticking or moving the cover glass, immerse the sample in 2xSSC for about 5S, take it out, gently push a corner of the cover glass to the edge of the slide with tweezers, and gently remove the cover glass with tweezers;

2 Place the sample at 2XSSC room temperature for 1 min;

(3) Take out the slides and immerse in a preheated at 68°C 0.3% NP-40/0.4xSSC (Preparation of 0.3% NP-40/0.4xSSC: For 1L preparation,

take 3mL NP-40 and 20mL 20xSSC, dissolve fully, mix well, and use 1M NaOH to adjust the pH to 7.2) solution and wash for 2min.

(4) Take out the sample and immerse it in deionized water preheated at 37°C in advance for 1min; dry it naturally in the dark place.

#### 4. Counterstaining

The following operations should be performed in a darkroom

10µl DAPI compound dye is dropped in the hybridization area of the glass slide and immediately covered. The suitable filter is selected for glass slide observation under the fluorescence microscope.

#### 5. FISH results observation

Place the stained sections under a fluorescence microscope and the cells area is first confirmed under a low magnification objective (10x); under magnification objective (40x) a uniform cells distribution is observed; then the nucleus size uniformity, nuclear boundary integrity, DAPI staining uniformity, no nuclei overlapping, cells clear signal are observed in the high magnification objective (10x).



# Wuhan HealthCare Biotechnology Co., Ltd.


 Building #8, Optics Valley Precision Medicine Industry Park Phase 1,

 #9 Gaokeyuan 3<sup>rd</sup> Road, East Lake High-Tech Zone. Zip Code 430206, Wuhan, Hubei, China.

 Tel#: +86(027)8757-0662 E-mail: cs@healthcare-biotech.com

 Website:

[Interpretation of common signal types]



### [Precautions]

(1) This product is only used for in vitro diagnosis.

2 The results of this kit will be affected by various factors of the sample itself, but also limited by hybridization temperature and time,

operating environment and the limitations of current molecular biology technology, which may lead to wrong results.

③ Users must understand the potential errors and accuracy limitations that may exist in the detection process.

(4) All chemicals are potentially dangerous. Avoid direct contact. Used kits are clinical waste and should be properly disposed of.

#### [Basic information]

Name of registrant / Manufacturer: Wuhan HealthCare Biotechnology Co., Ltd.

Address: Floor 1-4, Building #8, Optics Valley Precision Medicine Industry Base Phase I, #9 Gaokeyuan 3rd Road, East Lake High-Tech Zone, Wuhan City, Hubei Province, People's Republic of China.

Tel#: +86(027)8757-0662 E-mail: cs@healthcare-biotech.com | Website: www.healthcare-biotech.com

#### [Manual Approval date & Revision date]

V1. 0: Approval date: August 15, 2020.

V1. 3: Revision date: May 13, 2022.